

## Test report

Request No. : KATRM200323-033 Request date : 2020. 03. 23  
Report No. : KAAAM200408-012 Issue date : 2020. 04. 08  
Company : Jinnys Co., Ltd Purpose of use : Quality control  
Address : A-610, Cheonan mirae ace hightechcity, 10 Baekseokgongdan 1-ro, Seobuk-gu,  
Cheonan-si, Chungcheongnam-do, Republic of Korea (ZIOCODE: 31094)  
Person : Kim Sang Do  
Submit company :  
Name of sample : Acidic water using electrolysis of MEDIQA / MEDI@CIDIC ionizer

Test item	Test result	
	Control	Sample
Guidelines for evaluating external disinfectant efficacy		
<i>Staphylococcus aureus</i> ATCC 6538	Number of bacteria after 24 hr (CFU) 5.1 X 10 <sup>4</sup>	22
	Bacteria reduction rate (%)	99.9

※ Test method: *In vitro* method

※ Contact time: 24 hr


※ Bacterial reduction rate (%) = [(average CFU of control)-(average CFU of sample)]/(average CFU of control)X100

**Korea Analysis Test Researcher**




- Result picture -

ATCC 6538

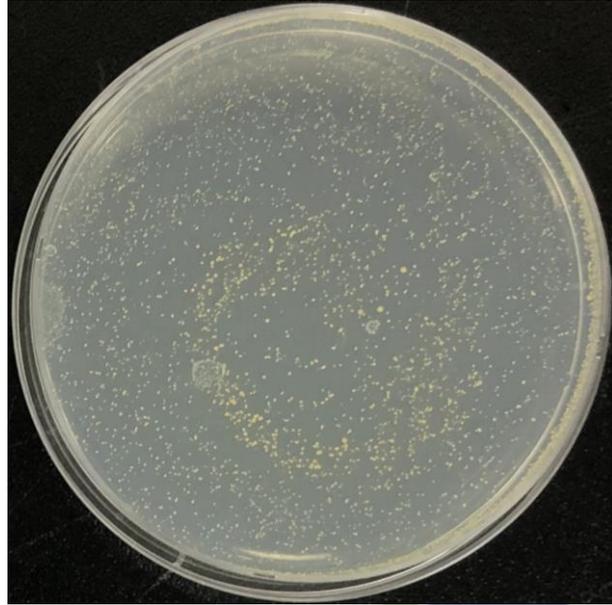

< Control >

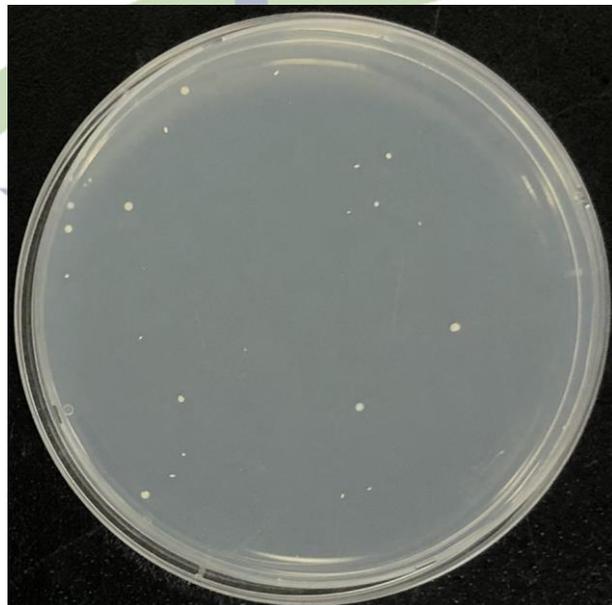

< Sample >

Remark: 1. This report is the result of test conducted by company's samples only. It does not guarantee the quality of all products.  
2. This report cannot be used for advertisement, campaign, and legal purpose without KATR's permission. Do not use for any other purposes.